

FIG. 1

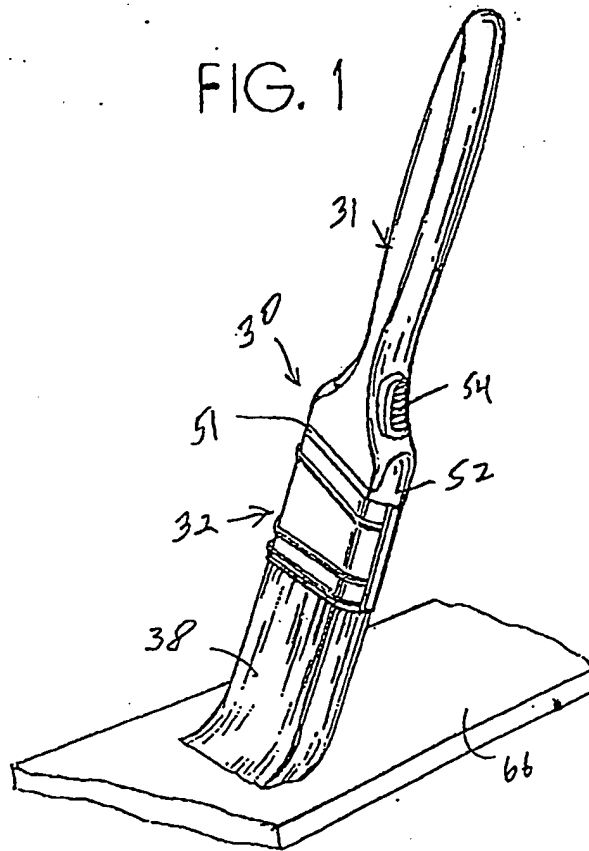
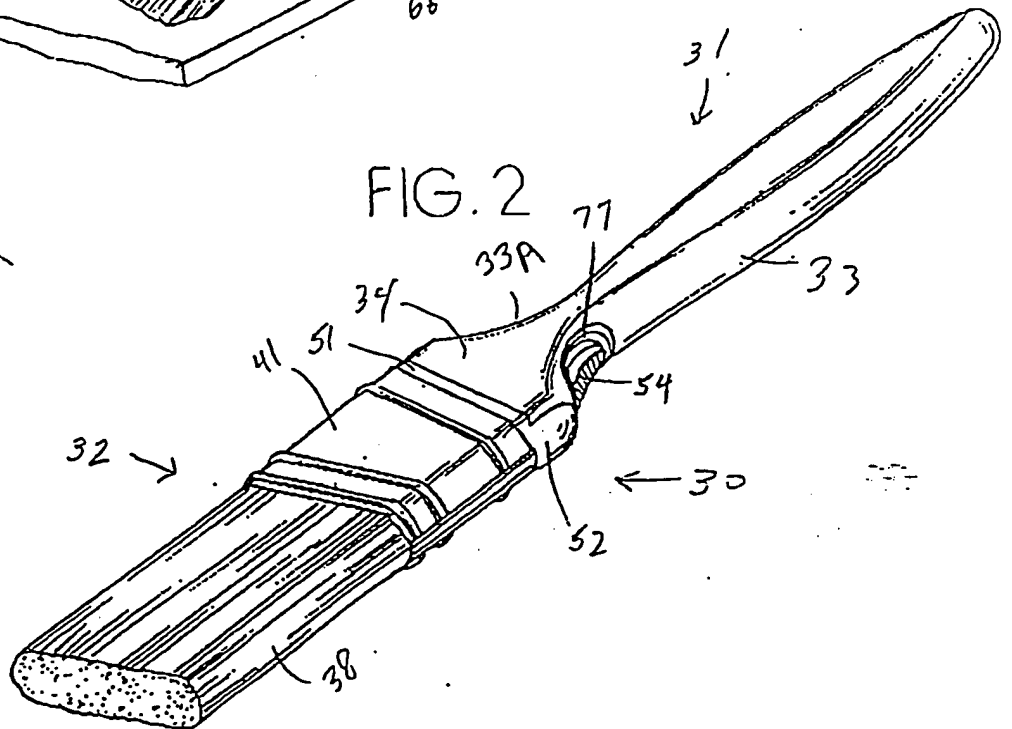
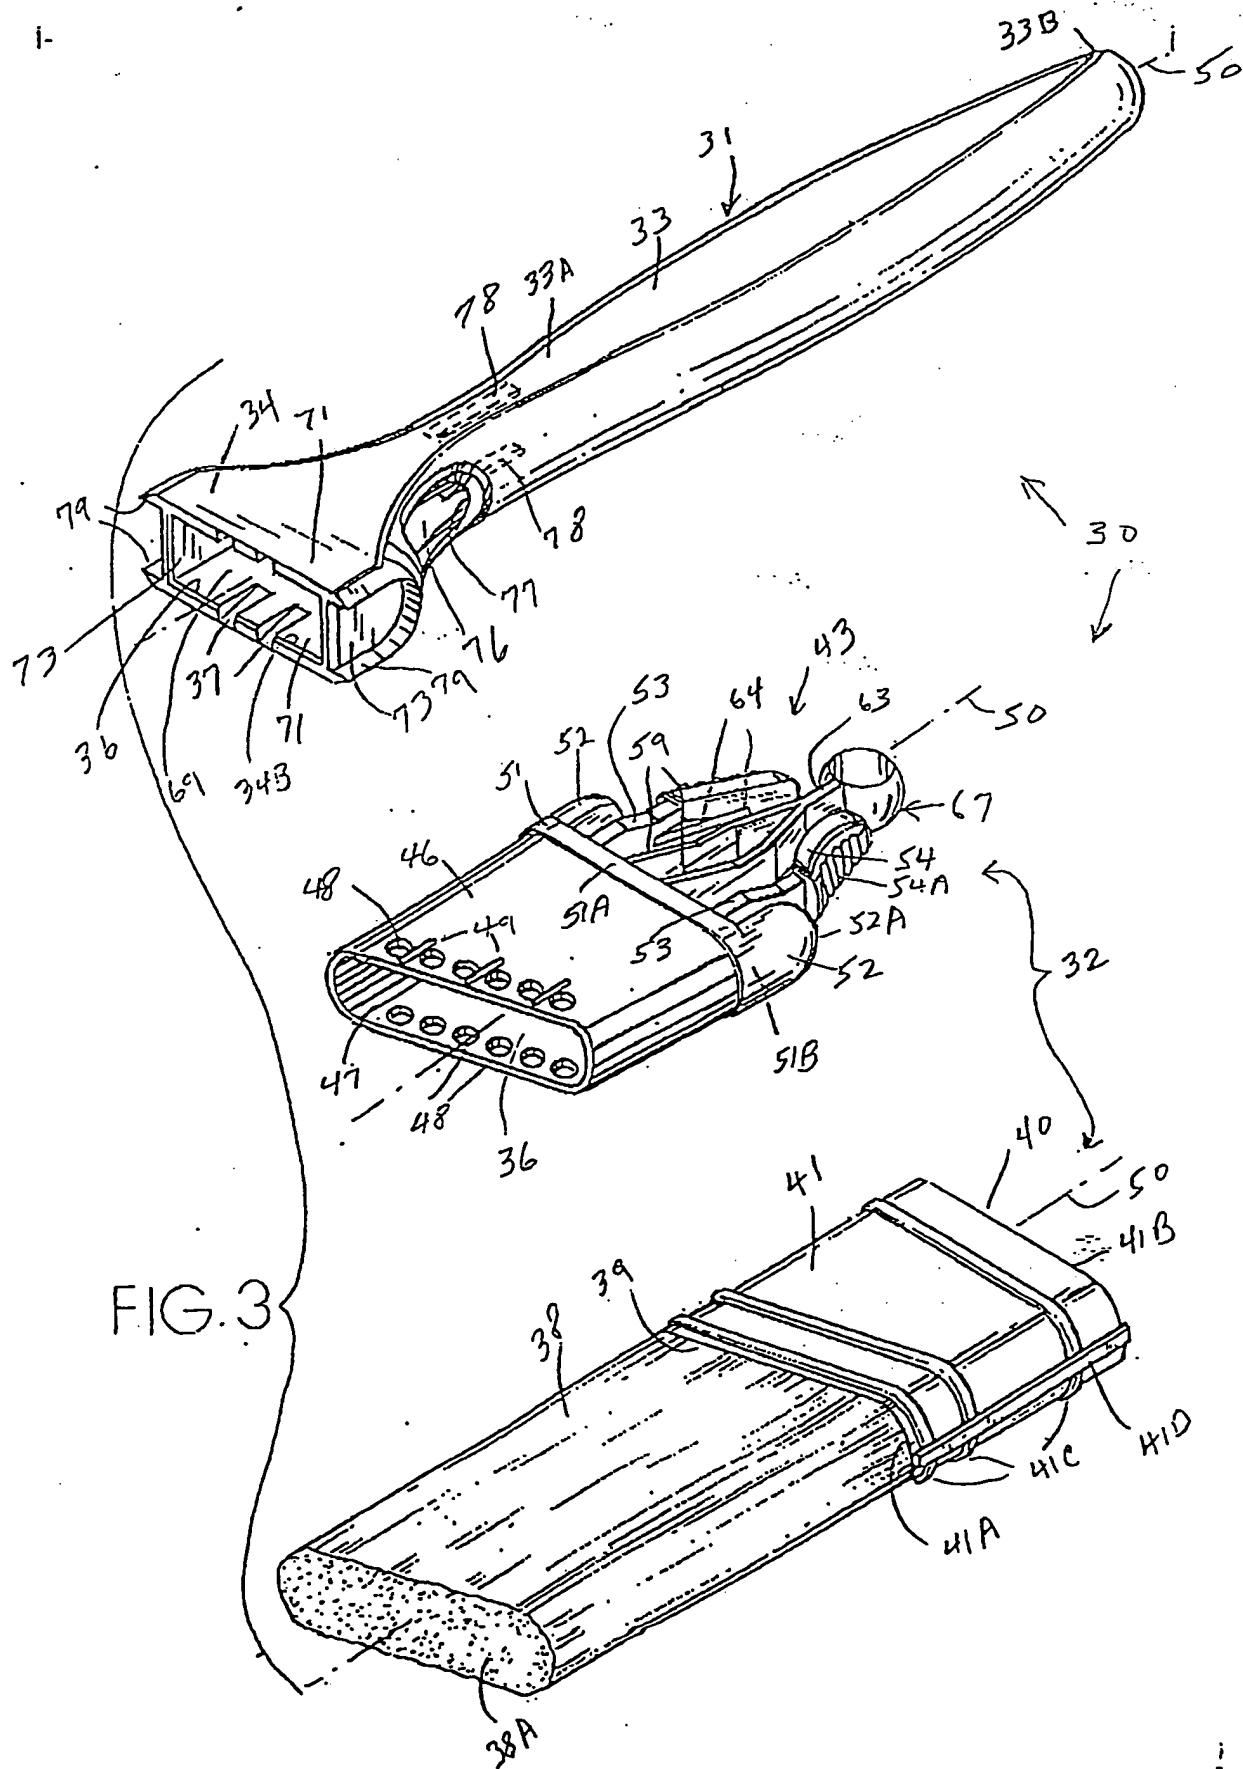


FIG. 2





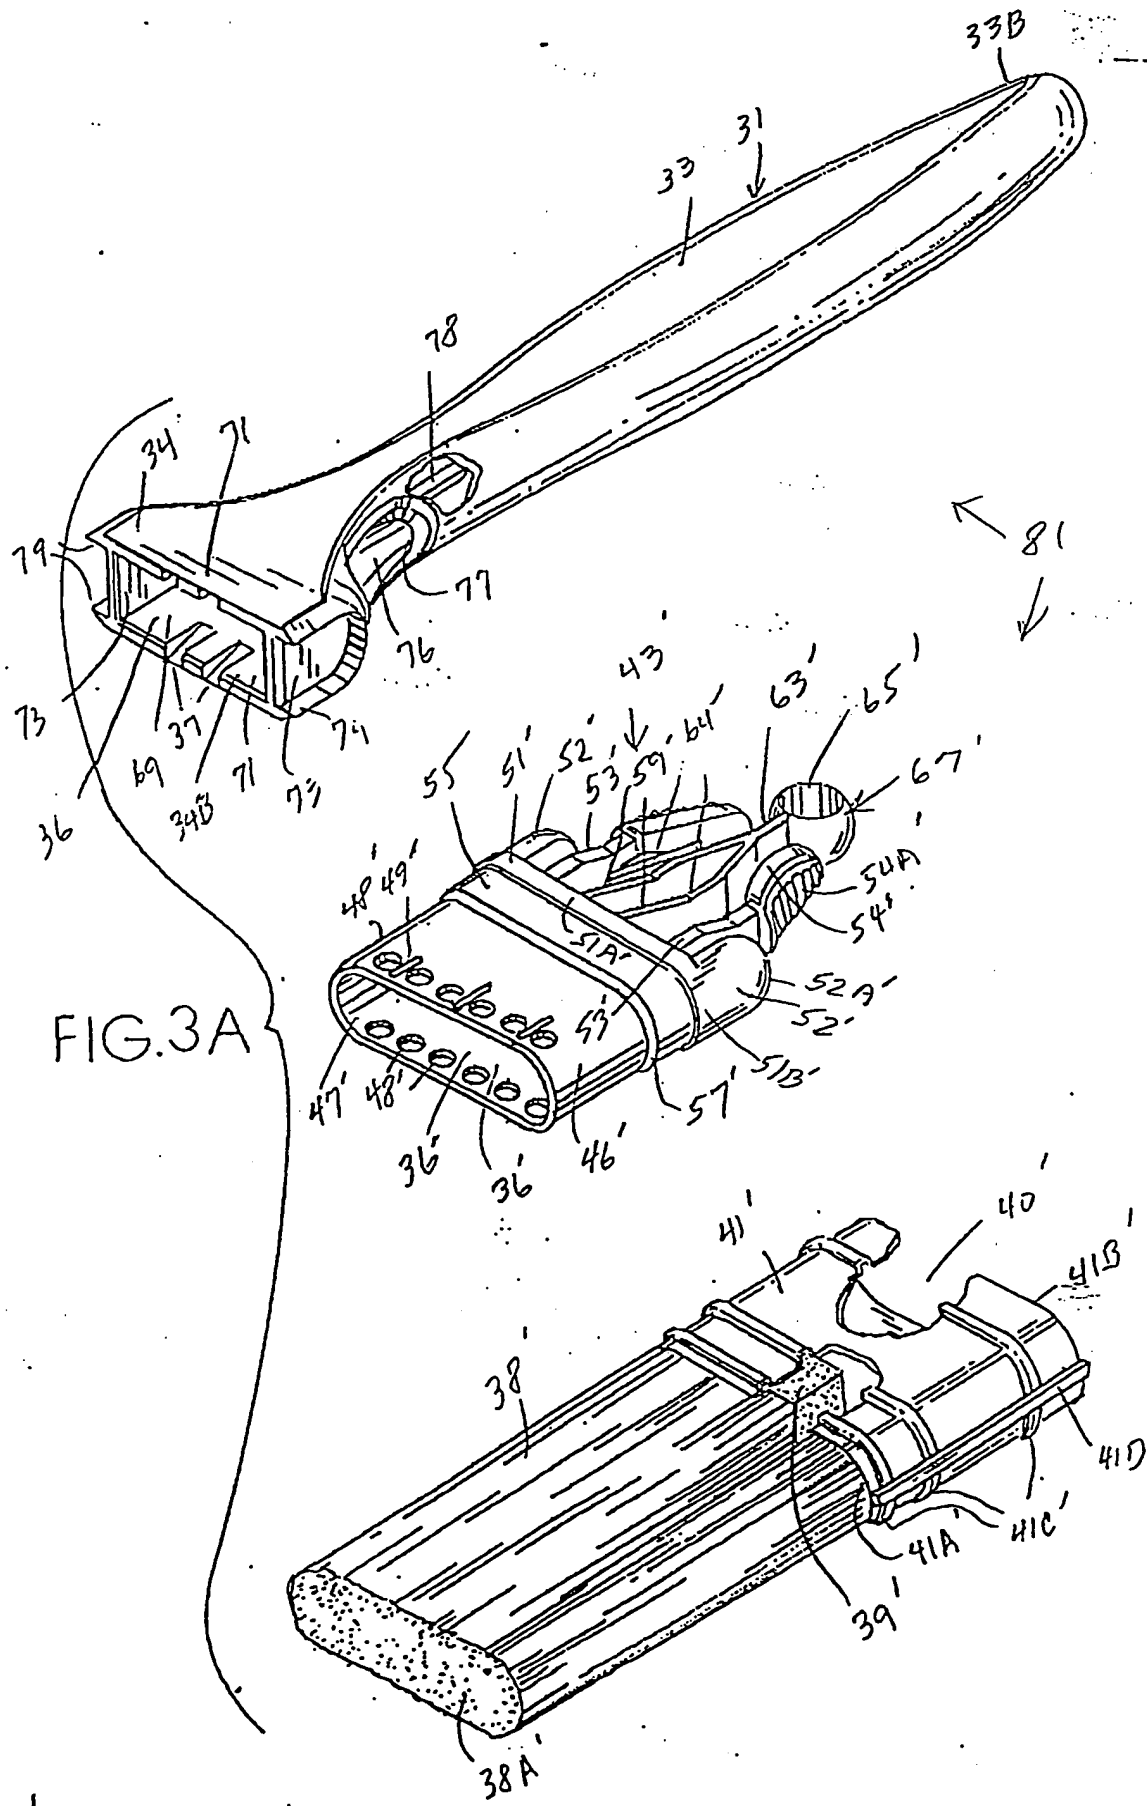


FIG. 4

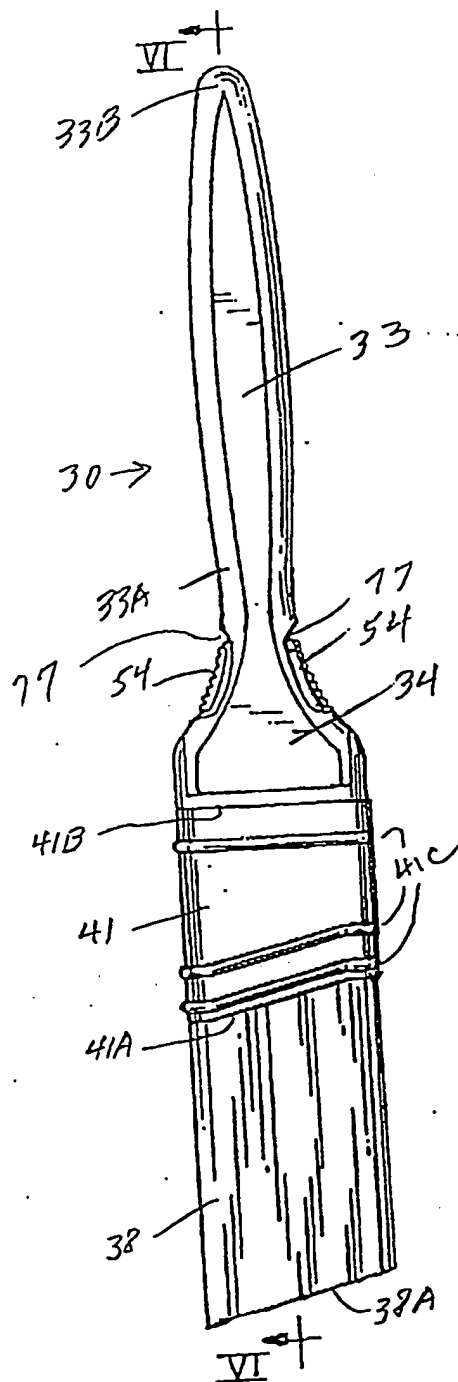


FIG. 5

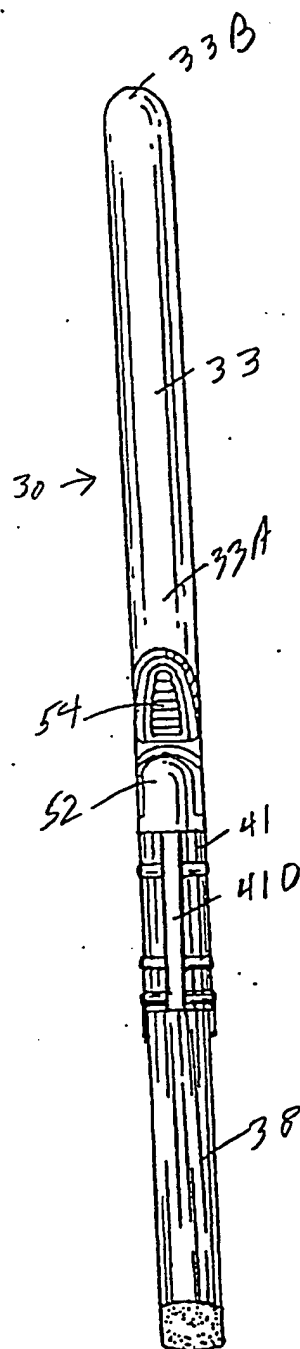


FIG. 6

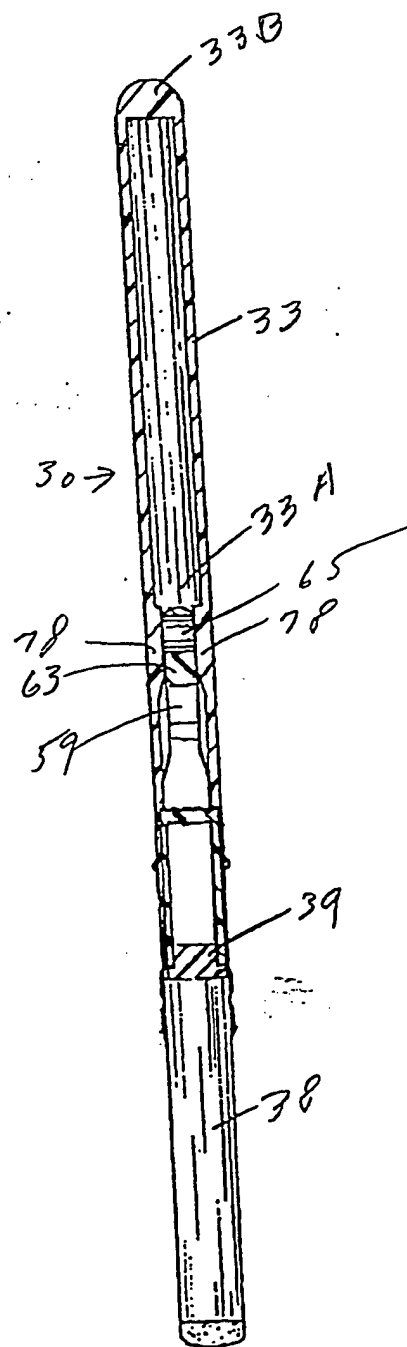


FIG. 7

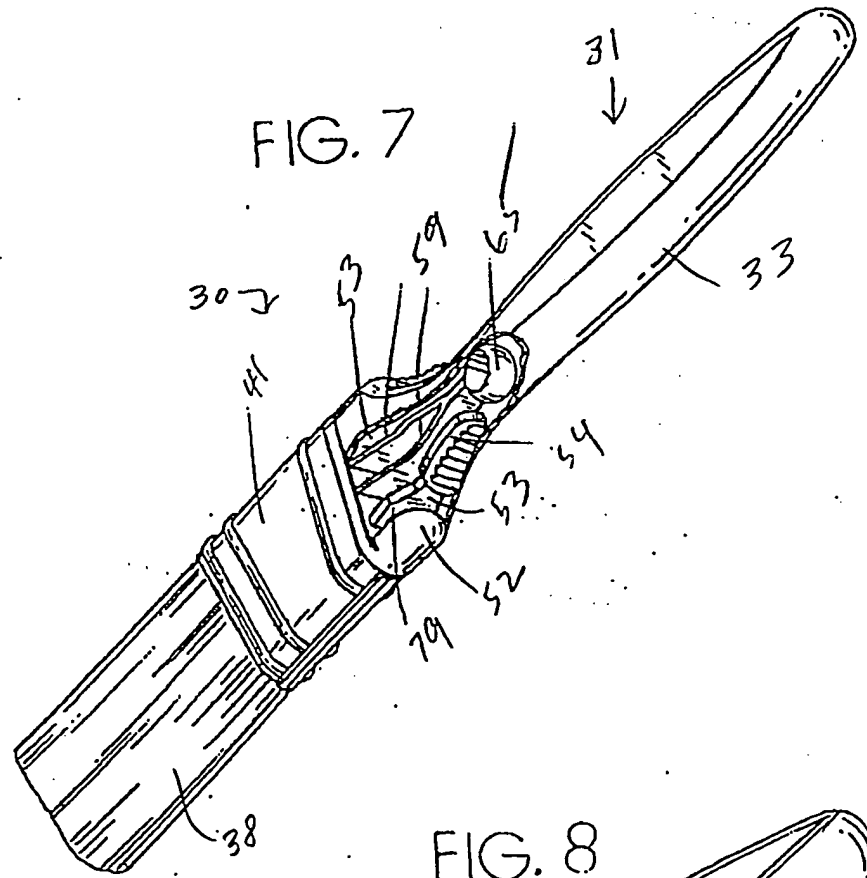
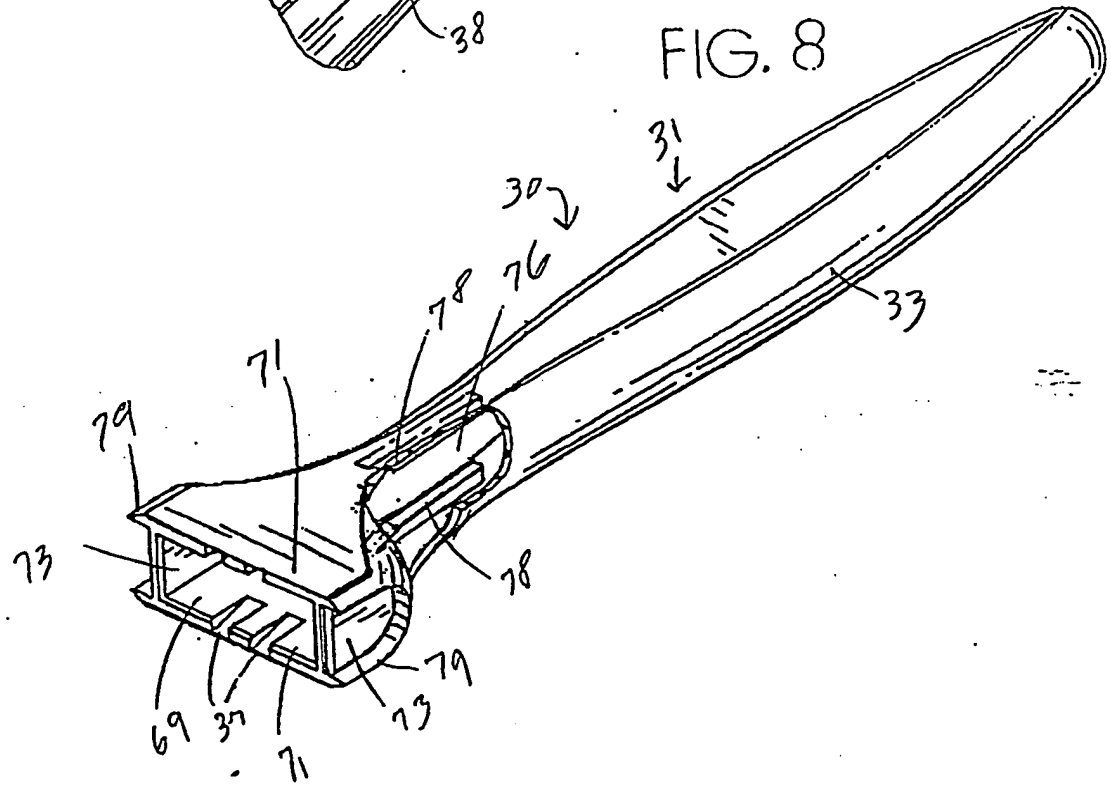
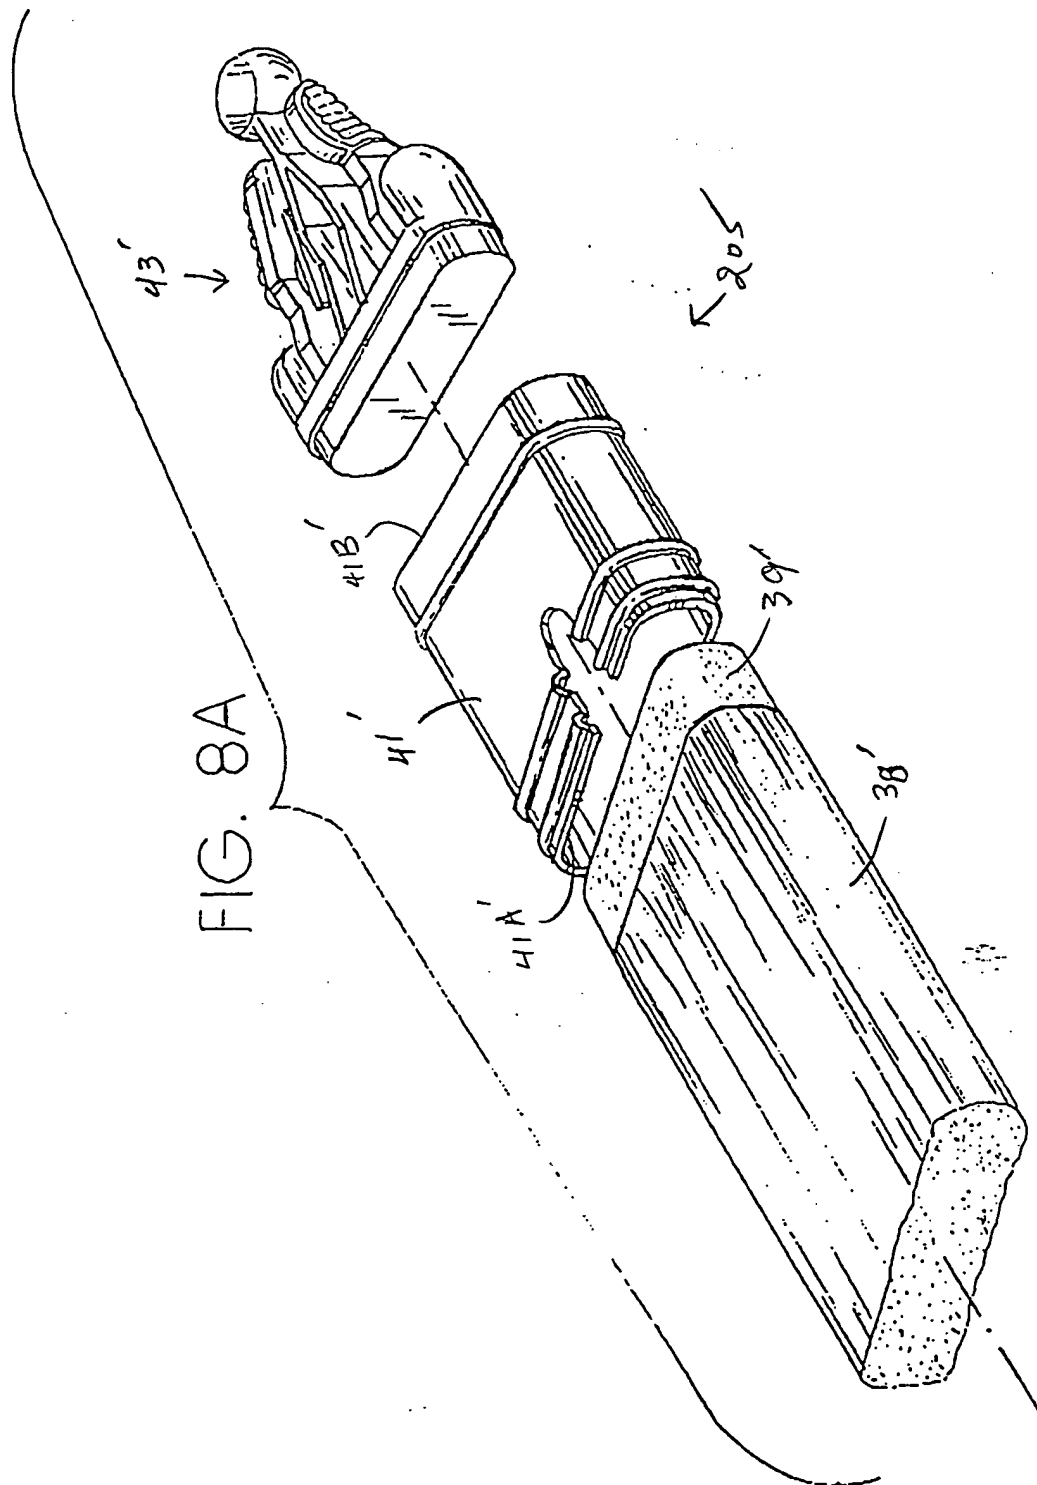
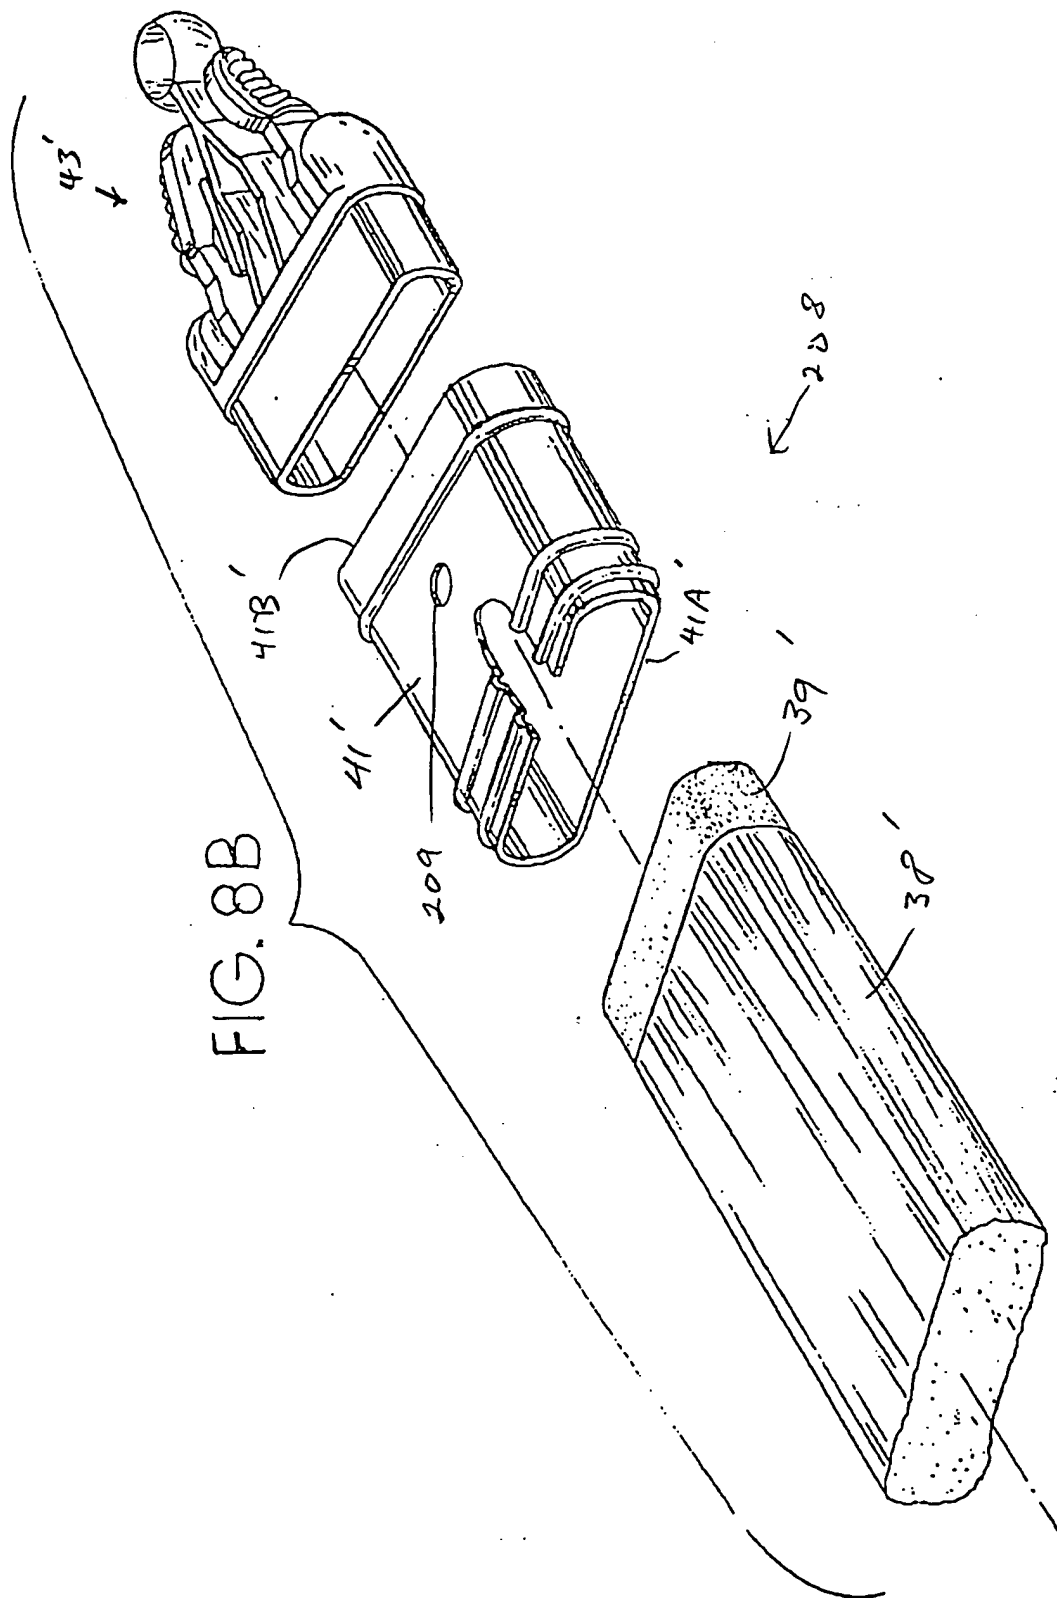
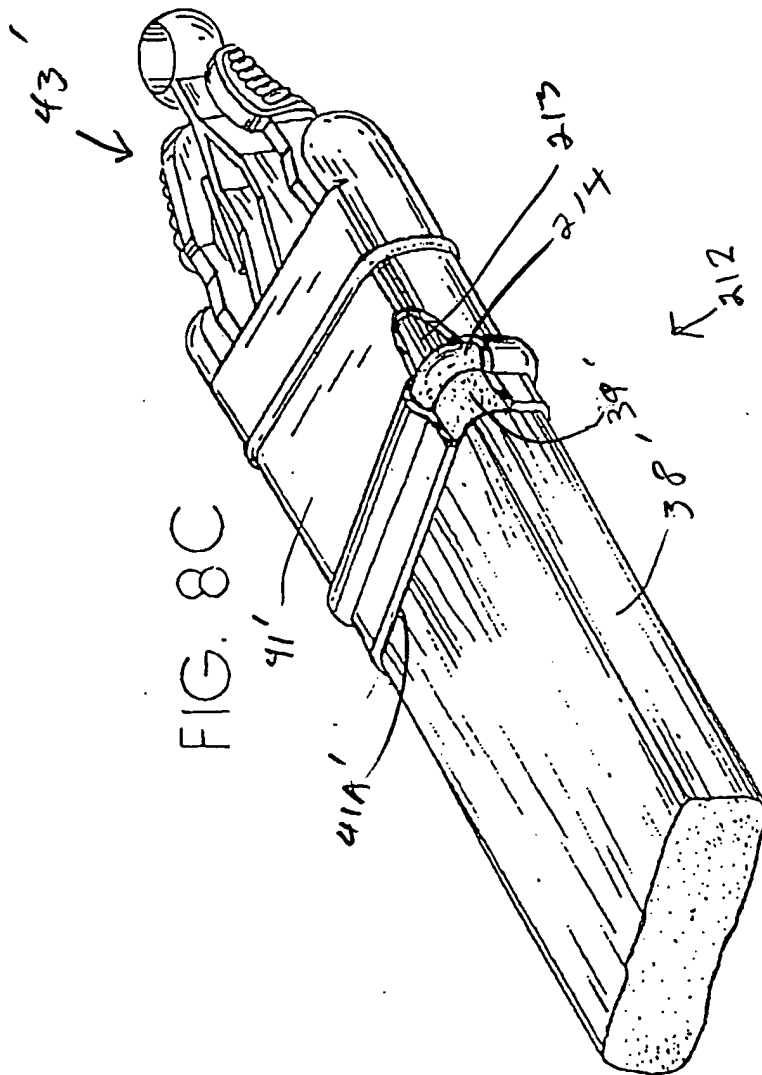


FIG. 8











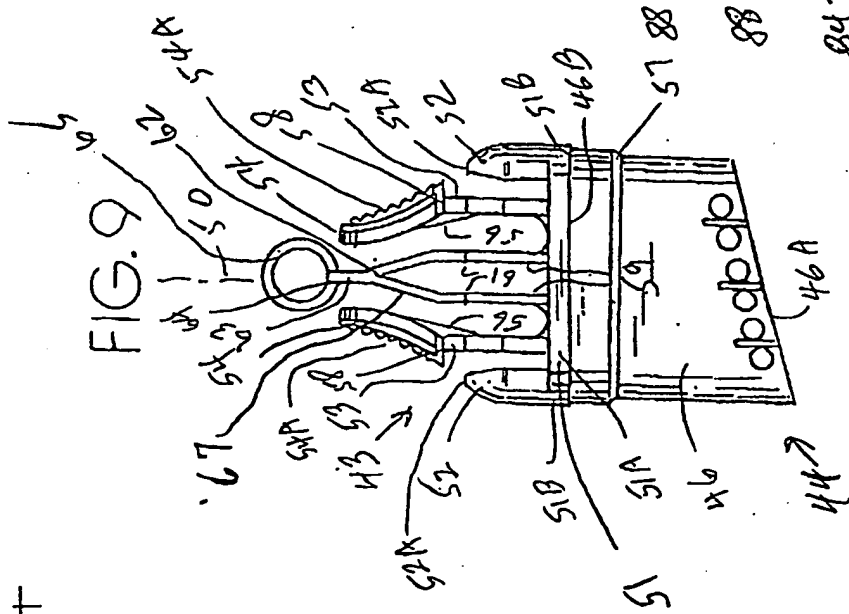


FIG. 9

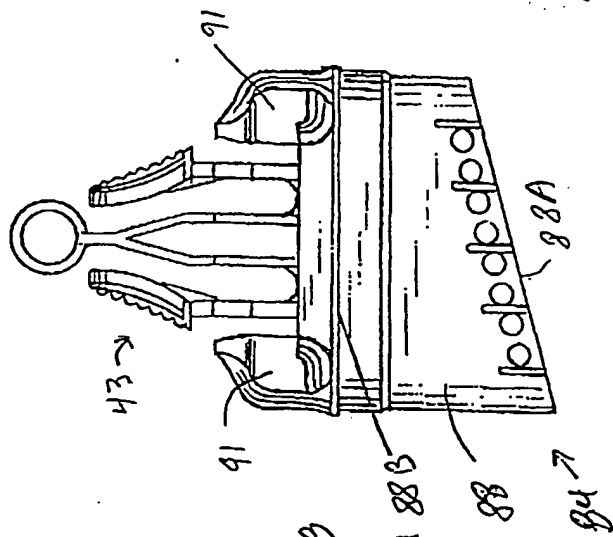


FIG. 10

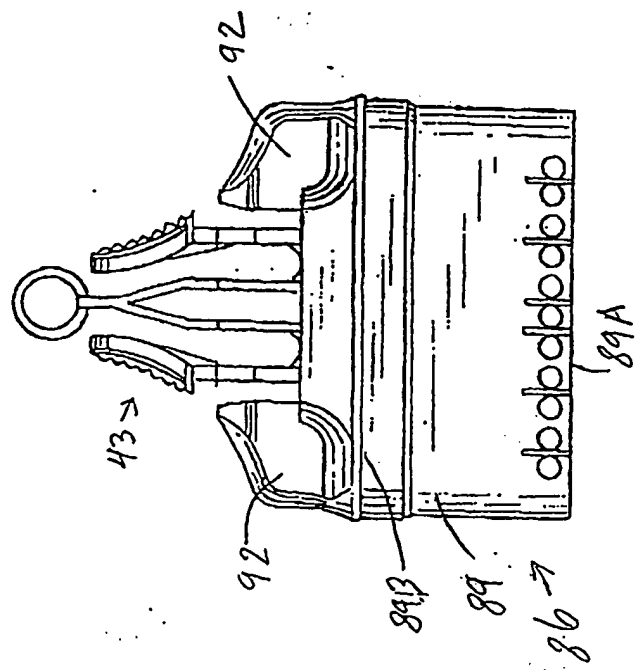


FIG. 11

FIG. 12

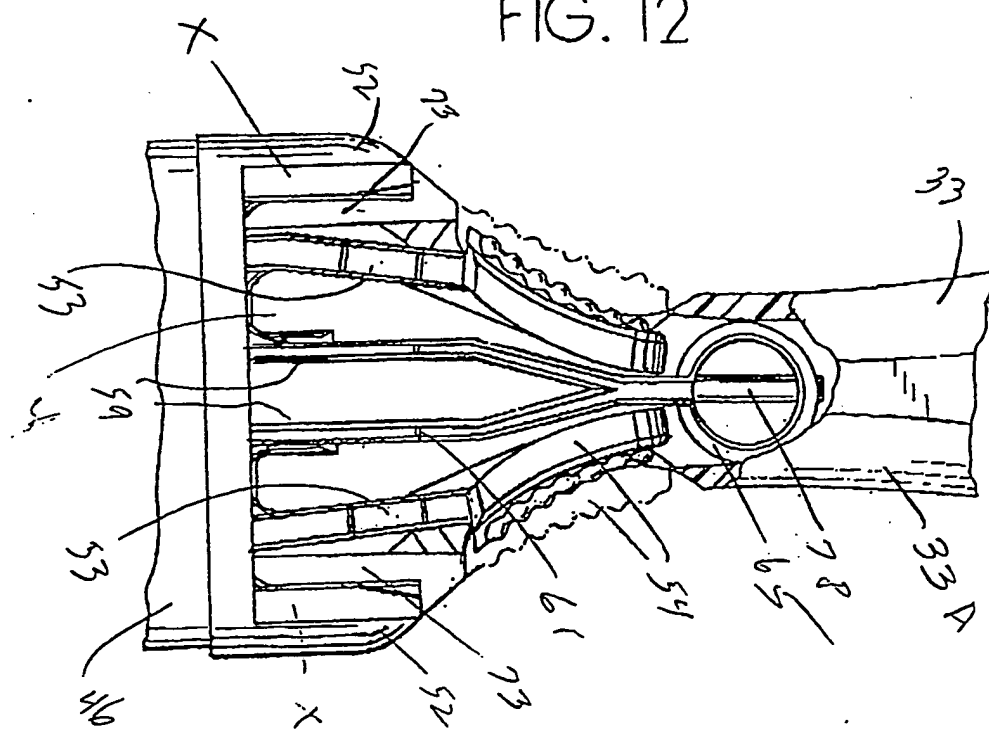


FIG. 13

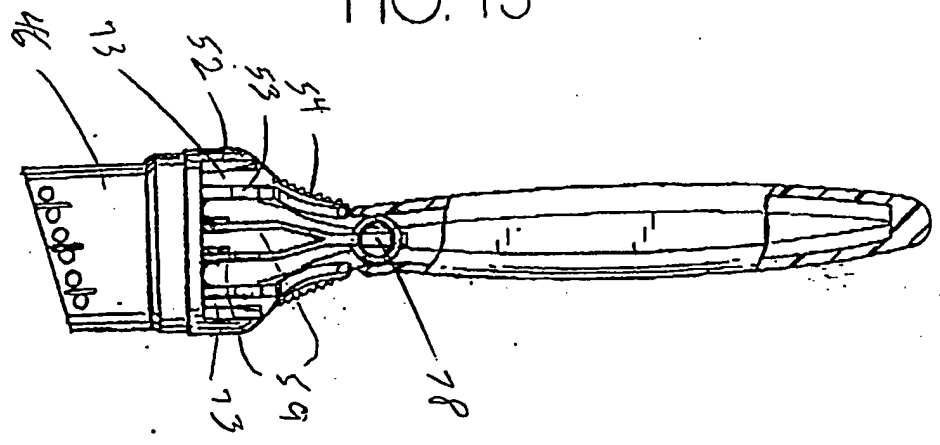


FIG. 12 is a cross-sectional view of the device taken along the line X-X of FIG. 13. FIG. 13 is a perspective view of the device.

FIG. 14

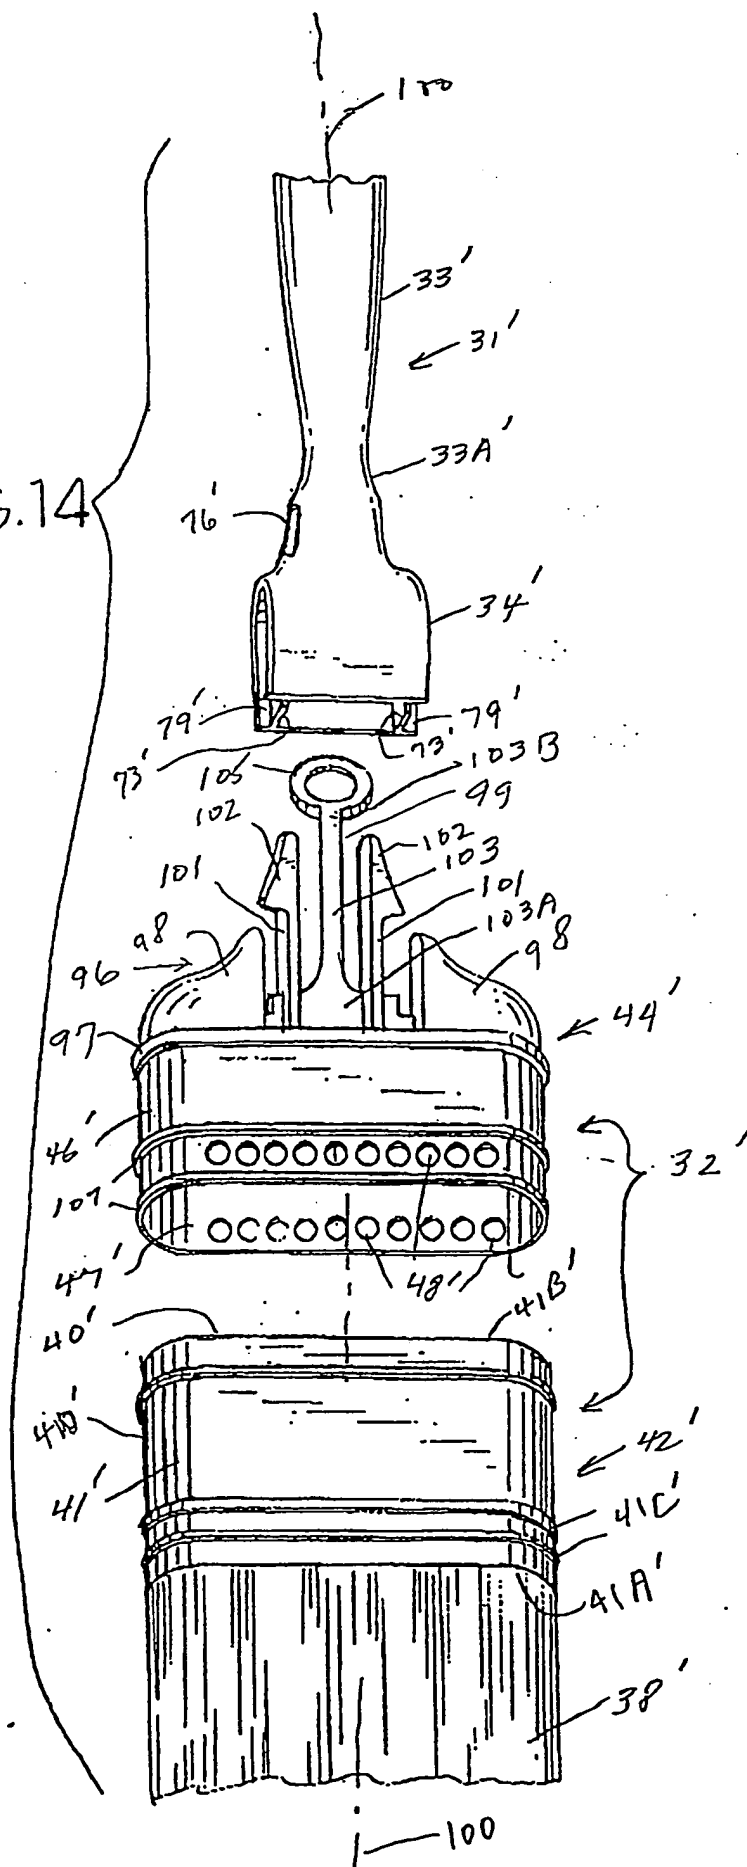


FIG. 15

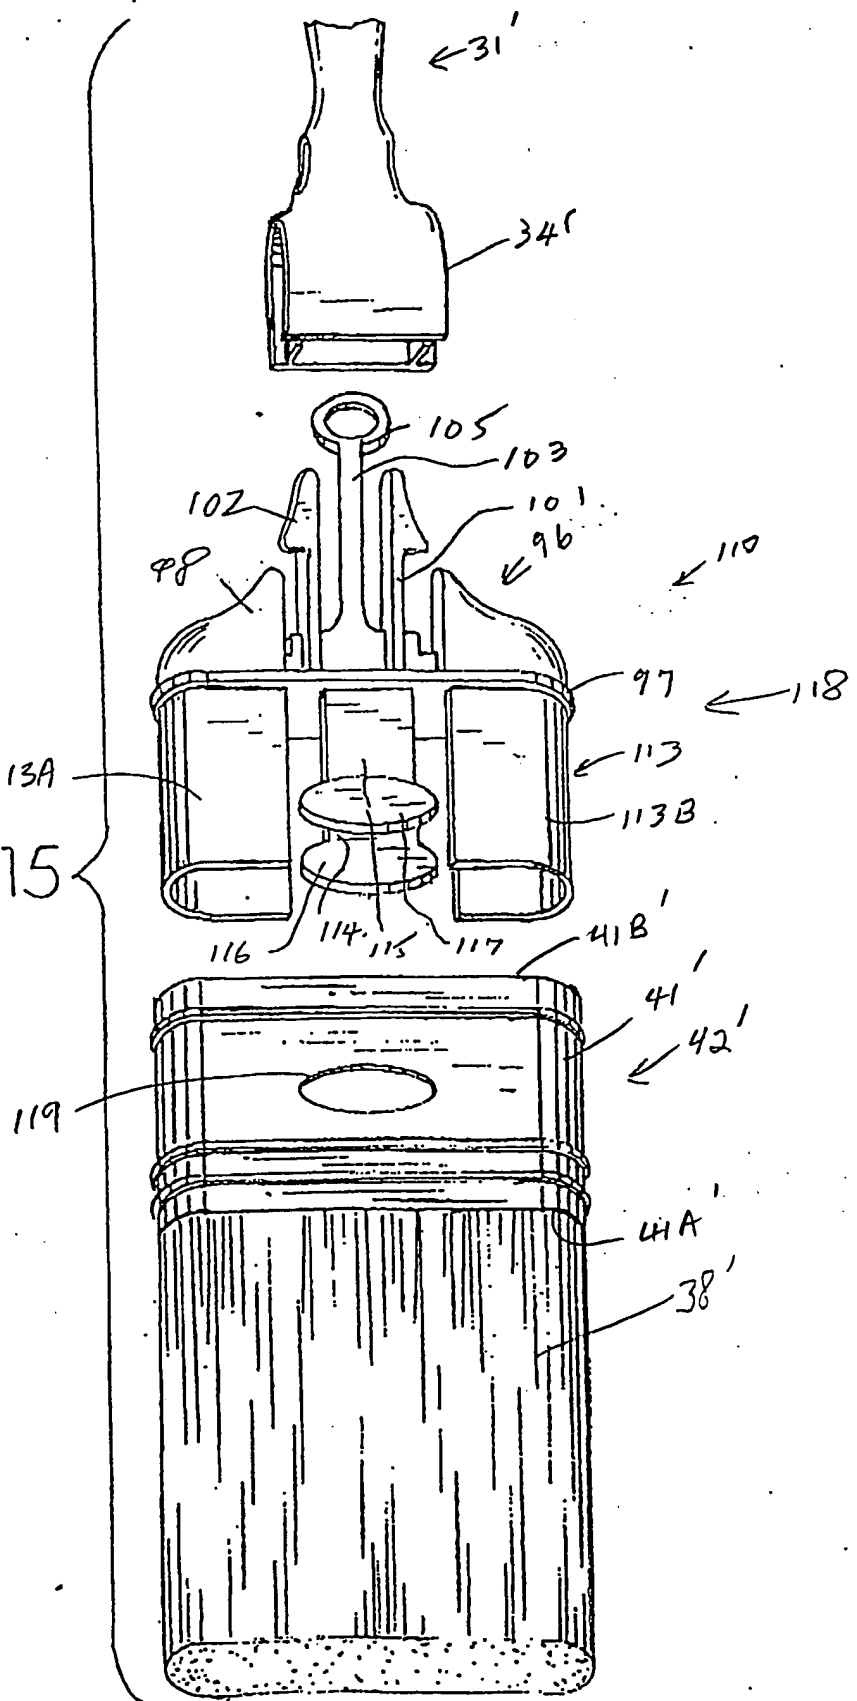
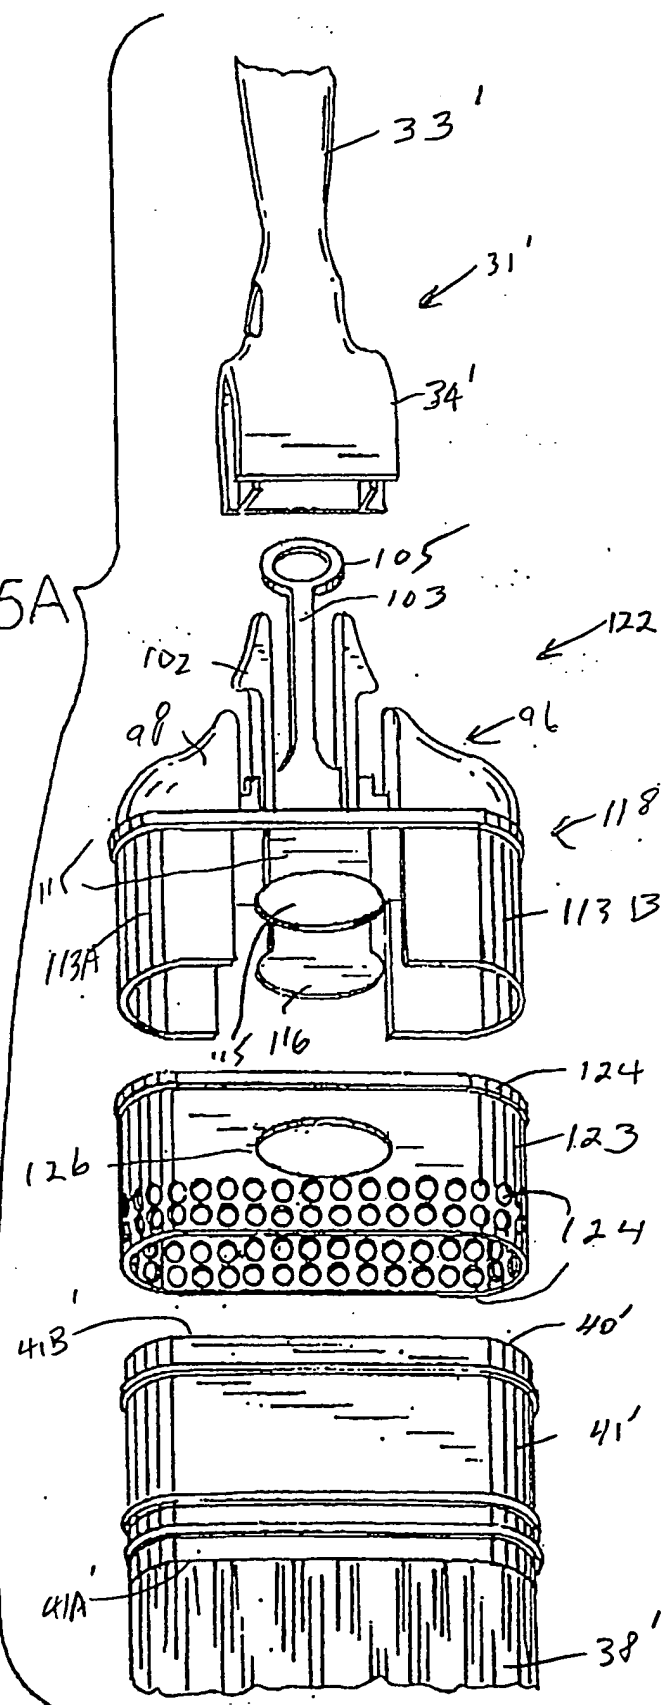


FIG. 15A



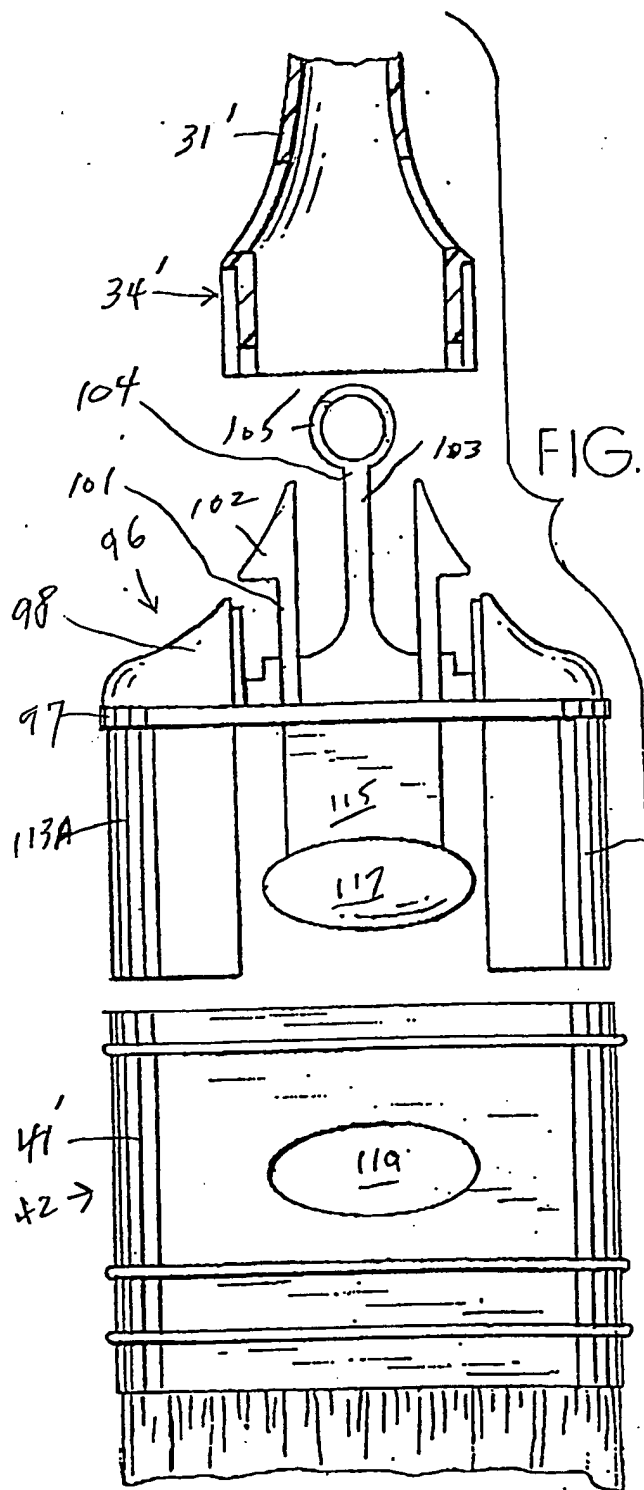


FIG. 16

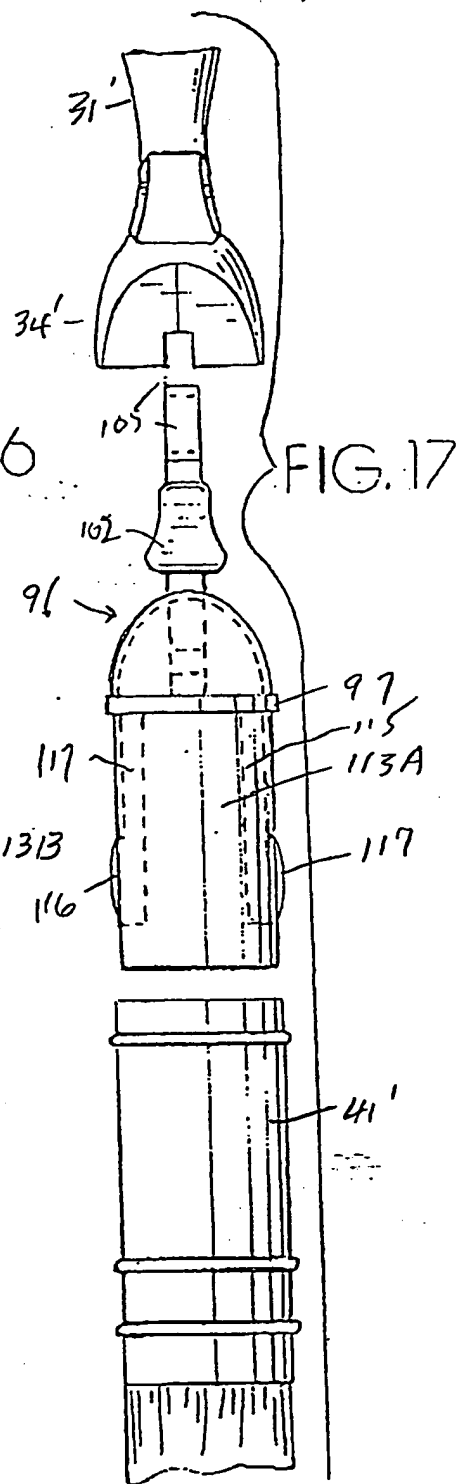


FIG. 17

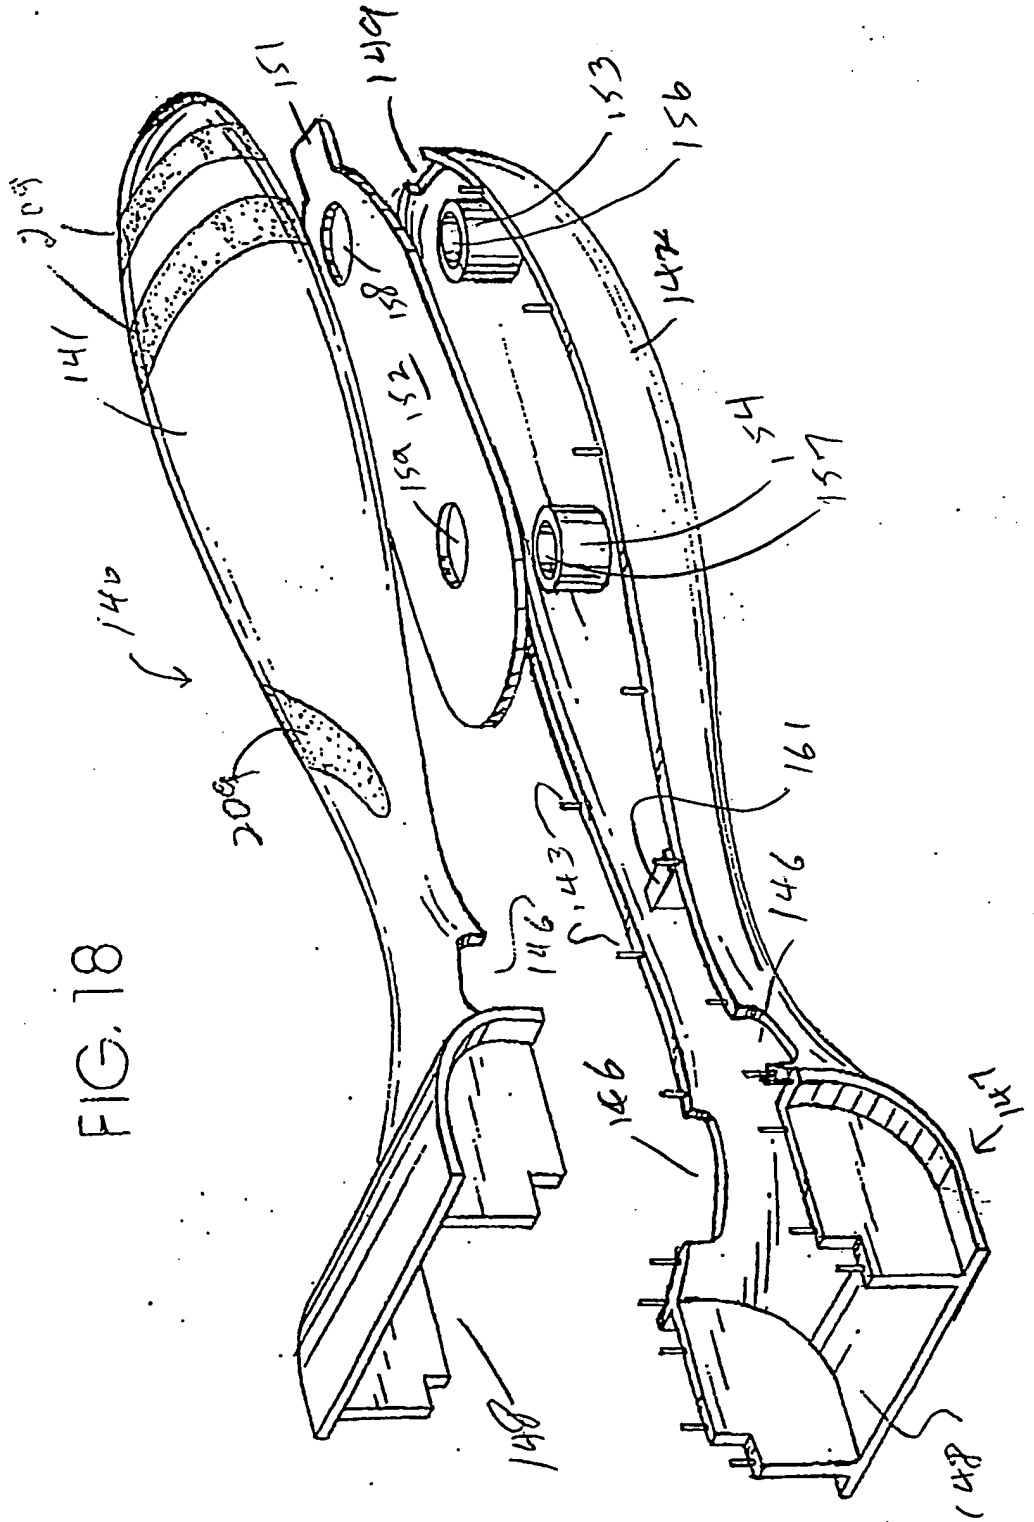


FIG. 19




FIG. 23




FIG. 20B

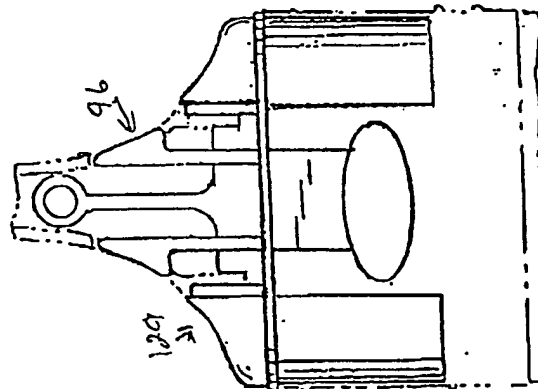


FIG. 20C

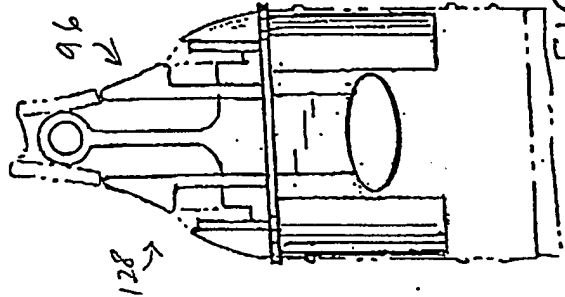


FIG. 22

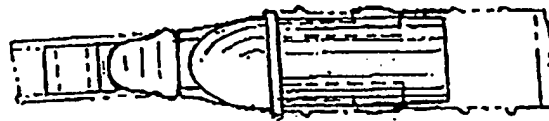


FIG. 21B



FIG. 21A







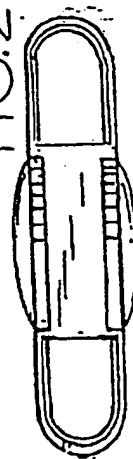


FIG. 21C

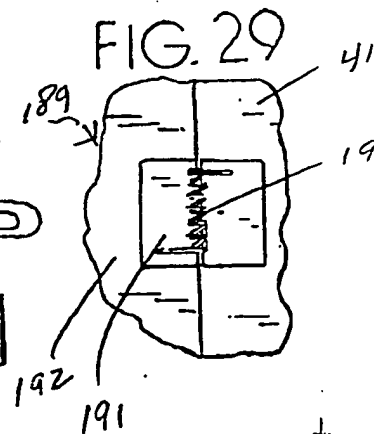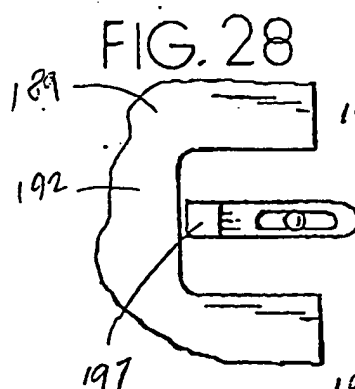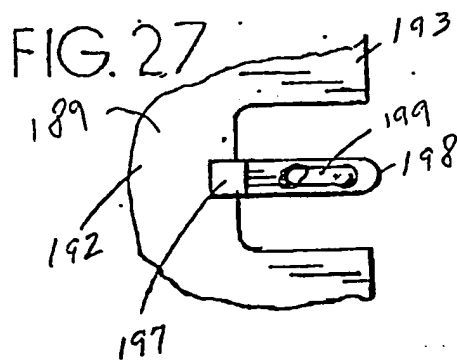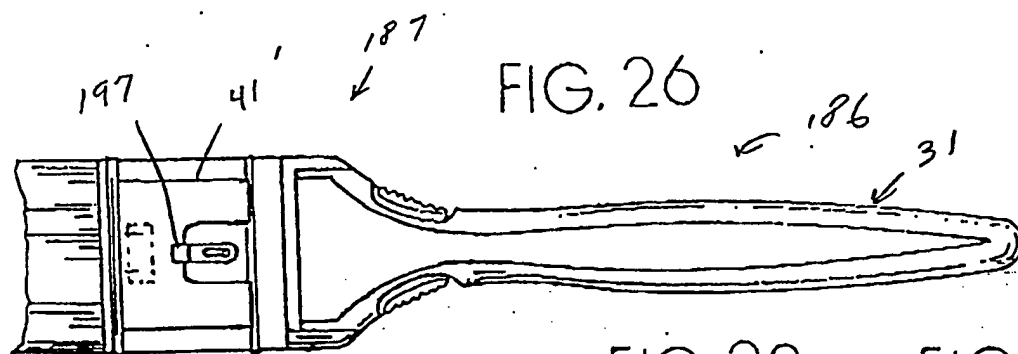

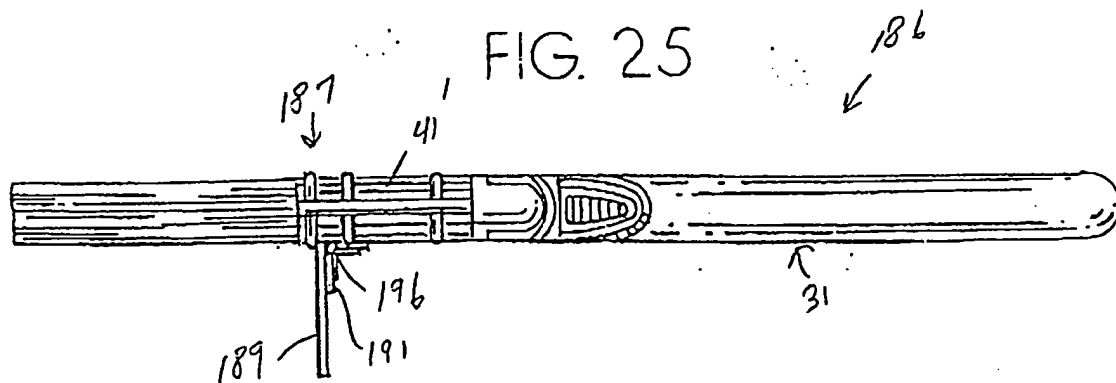

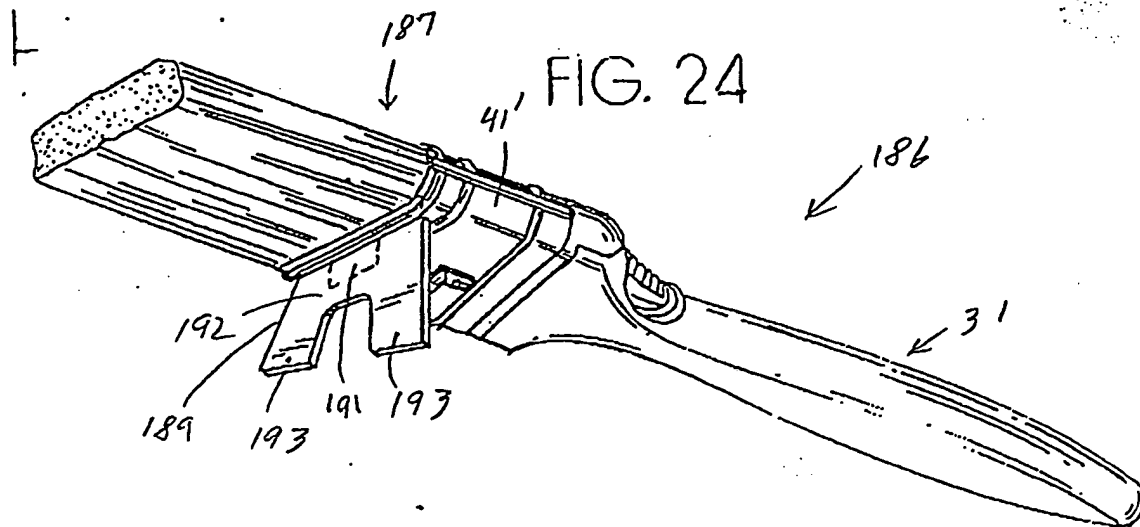

+

FIG. 30

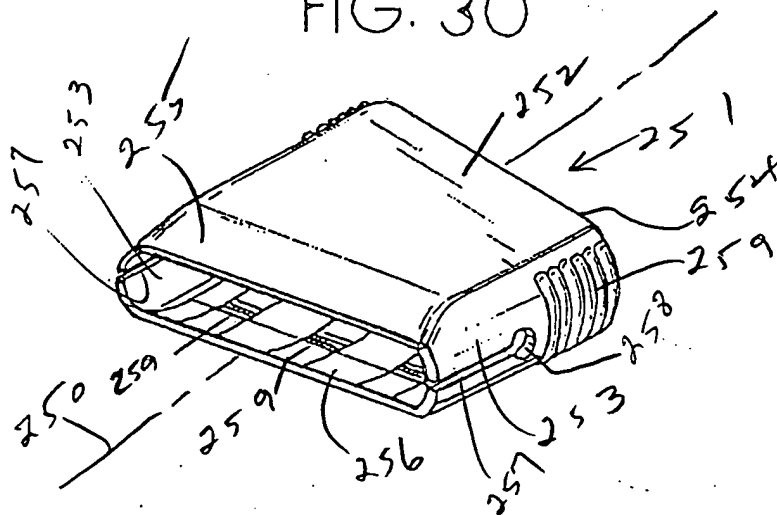


FIG. 31

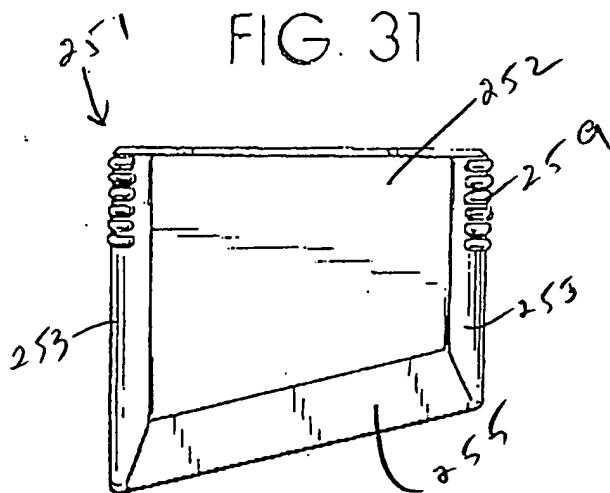


FIG. 32

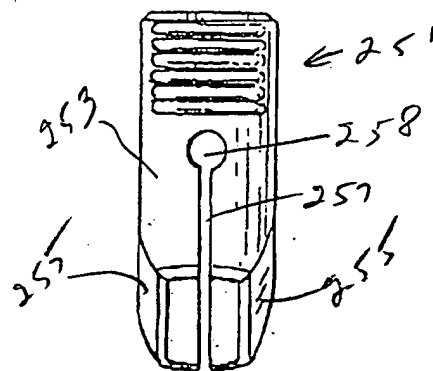


FIG. 36

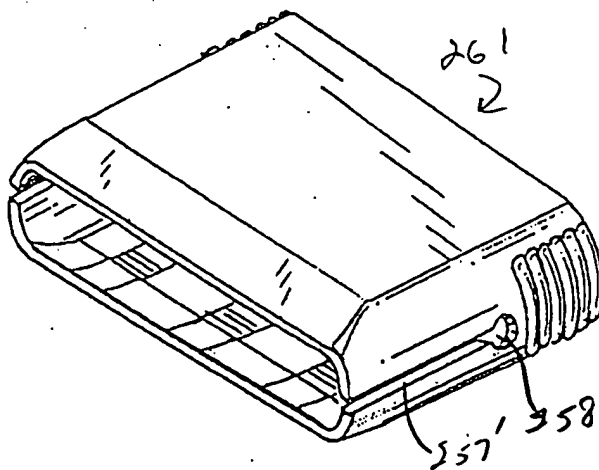
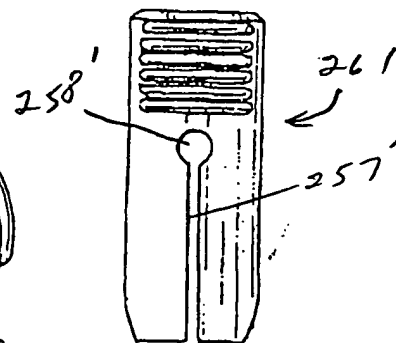


FIG. 37



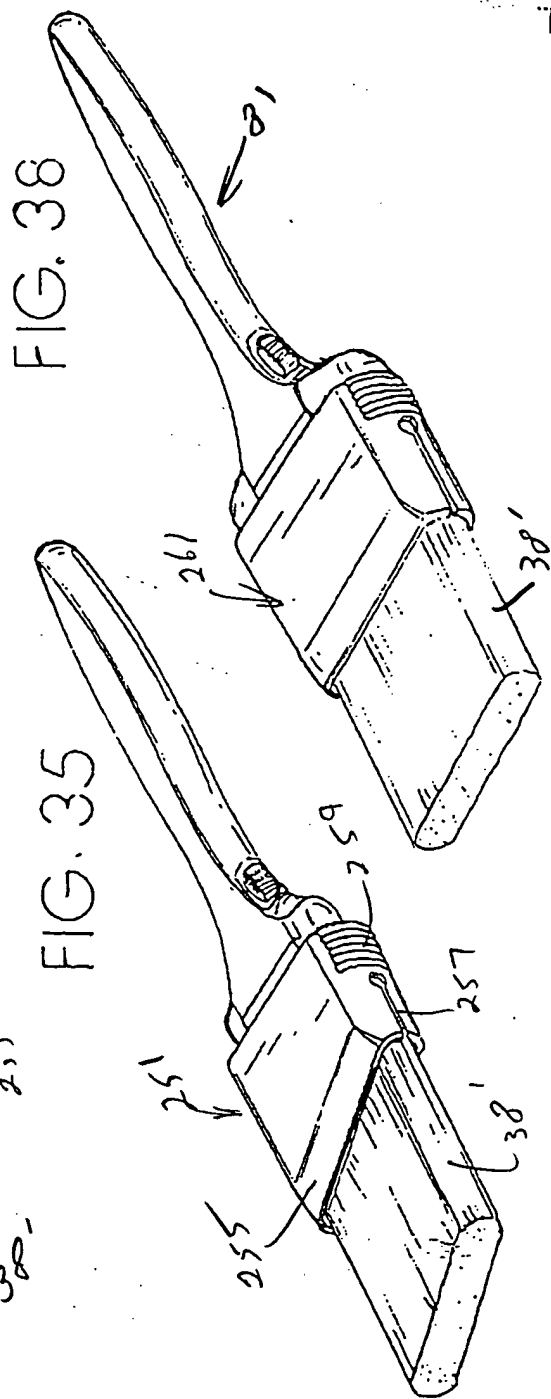
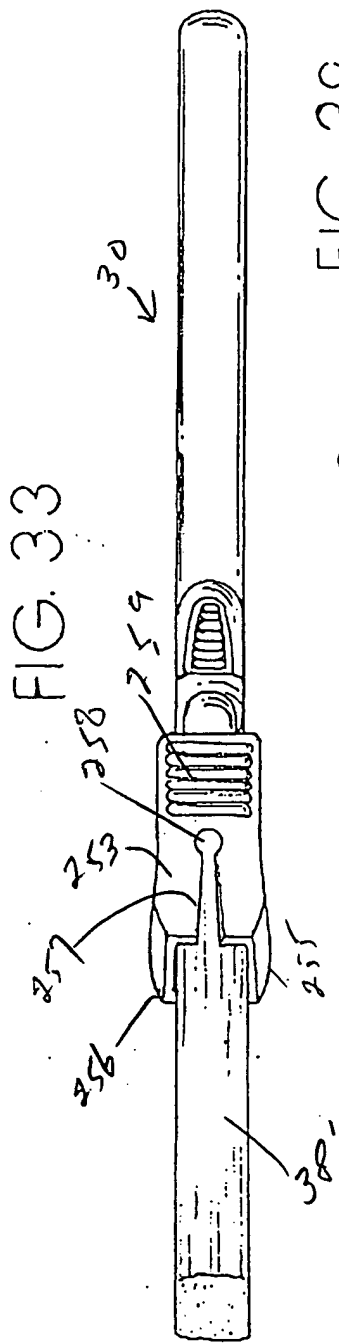
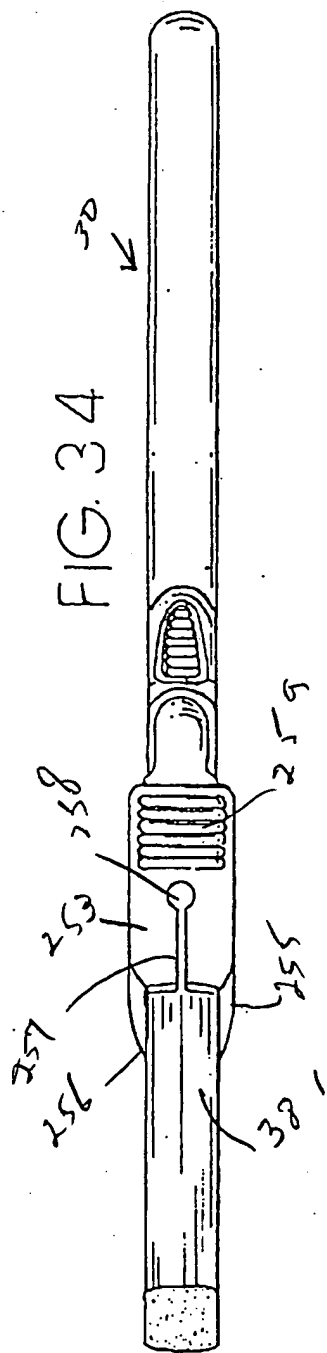


FIG. 39

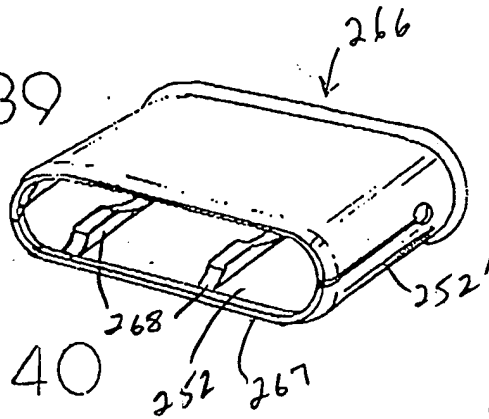


FIG. 40

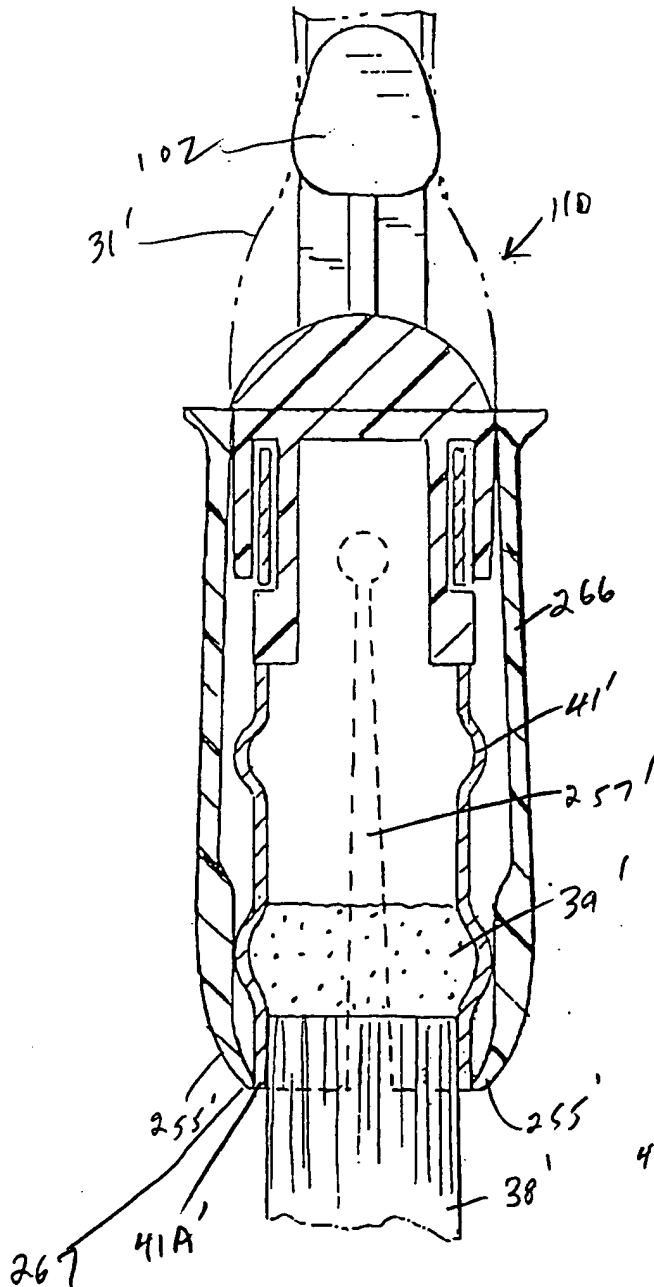
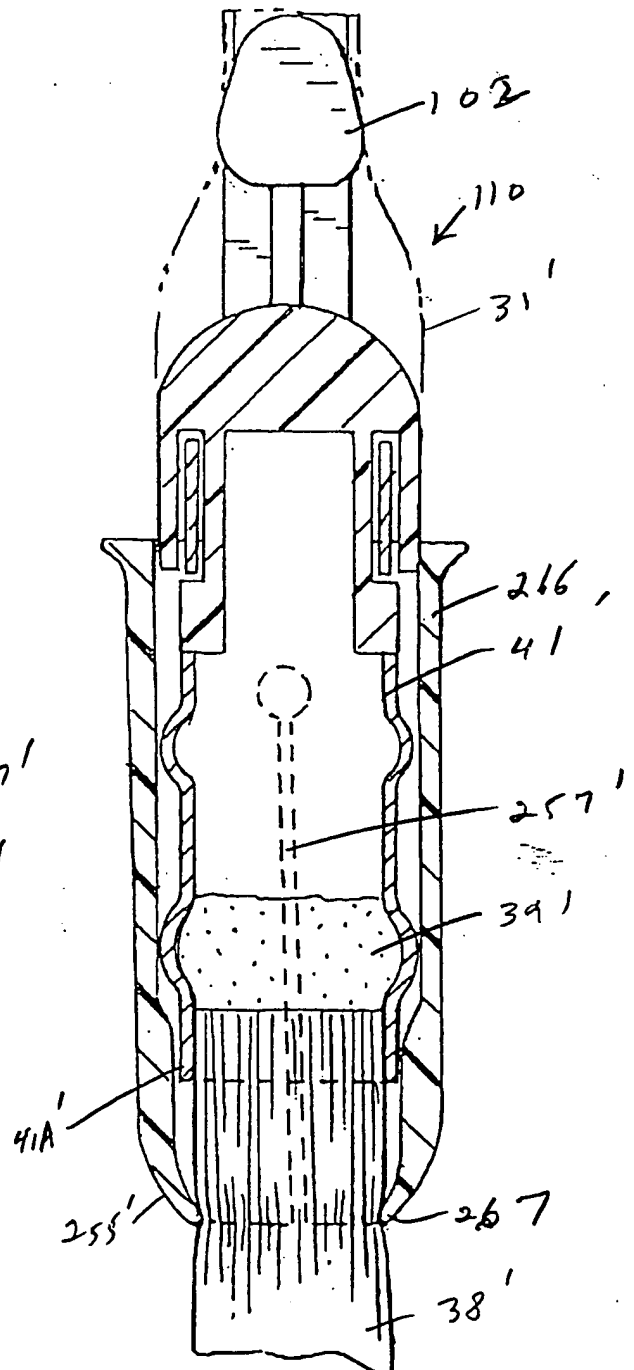


FIG. 41



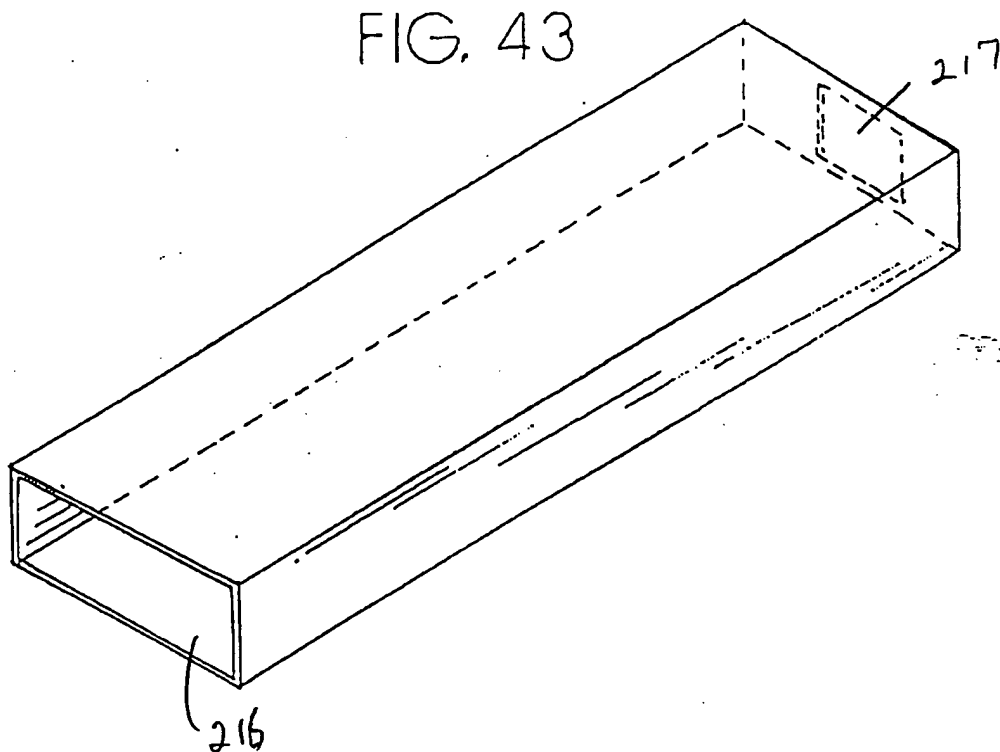
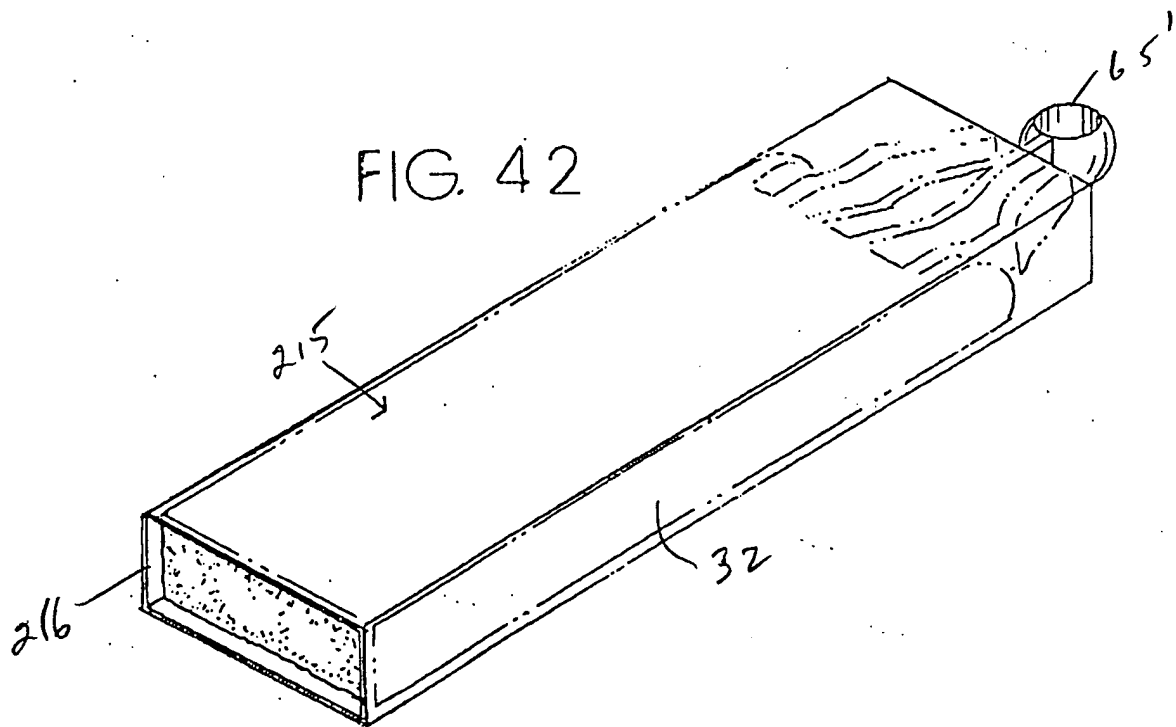


FIG. 44

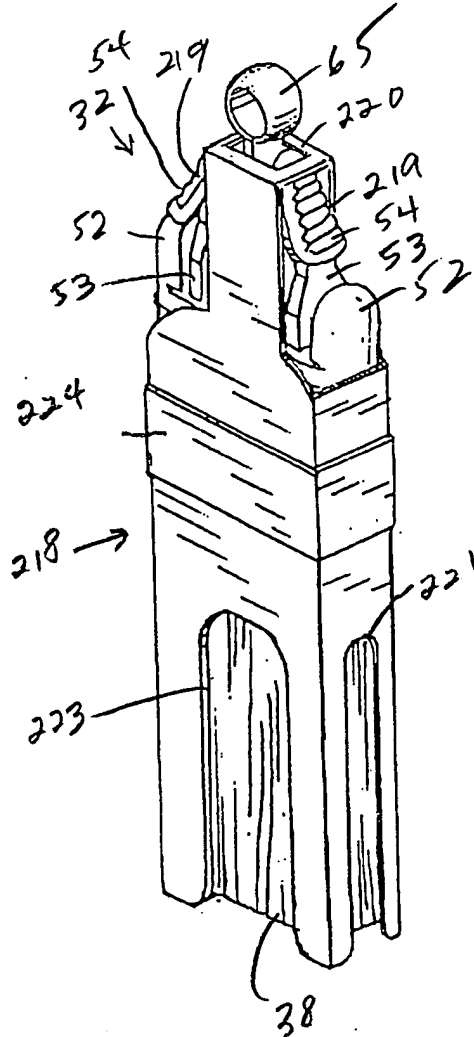


FIG. 46

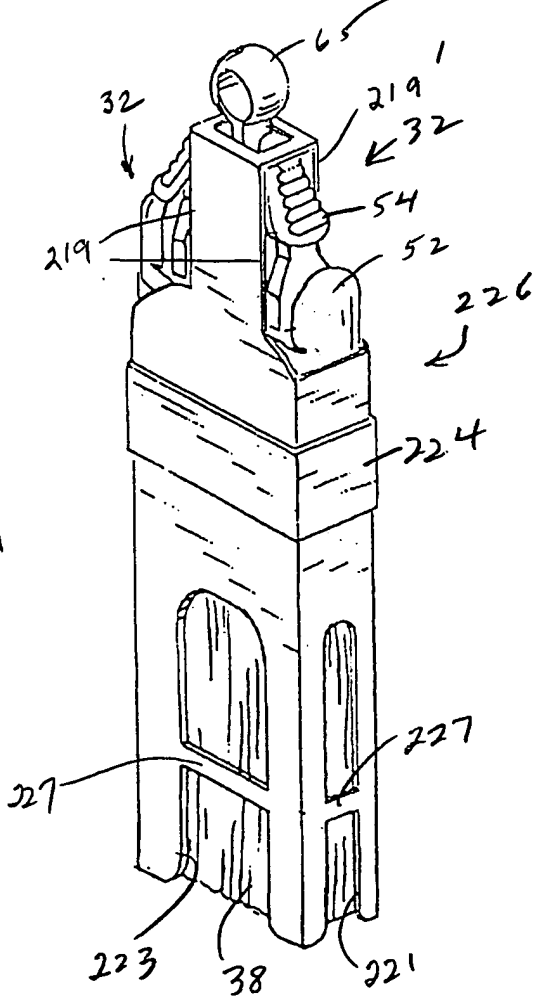


FIG. 45

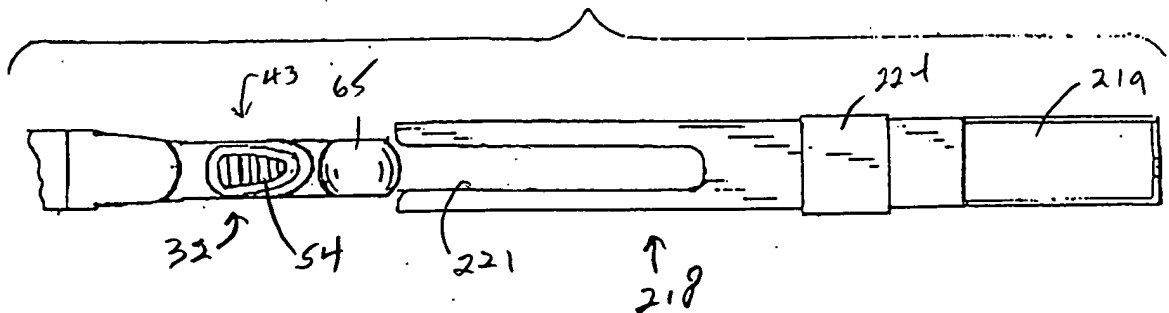


FIG. 47

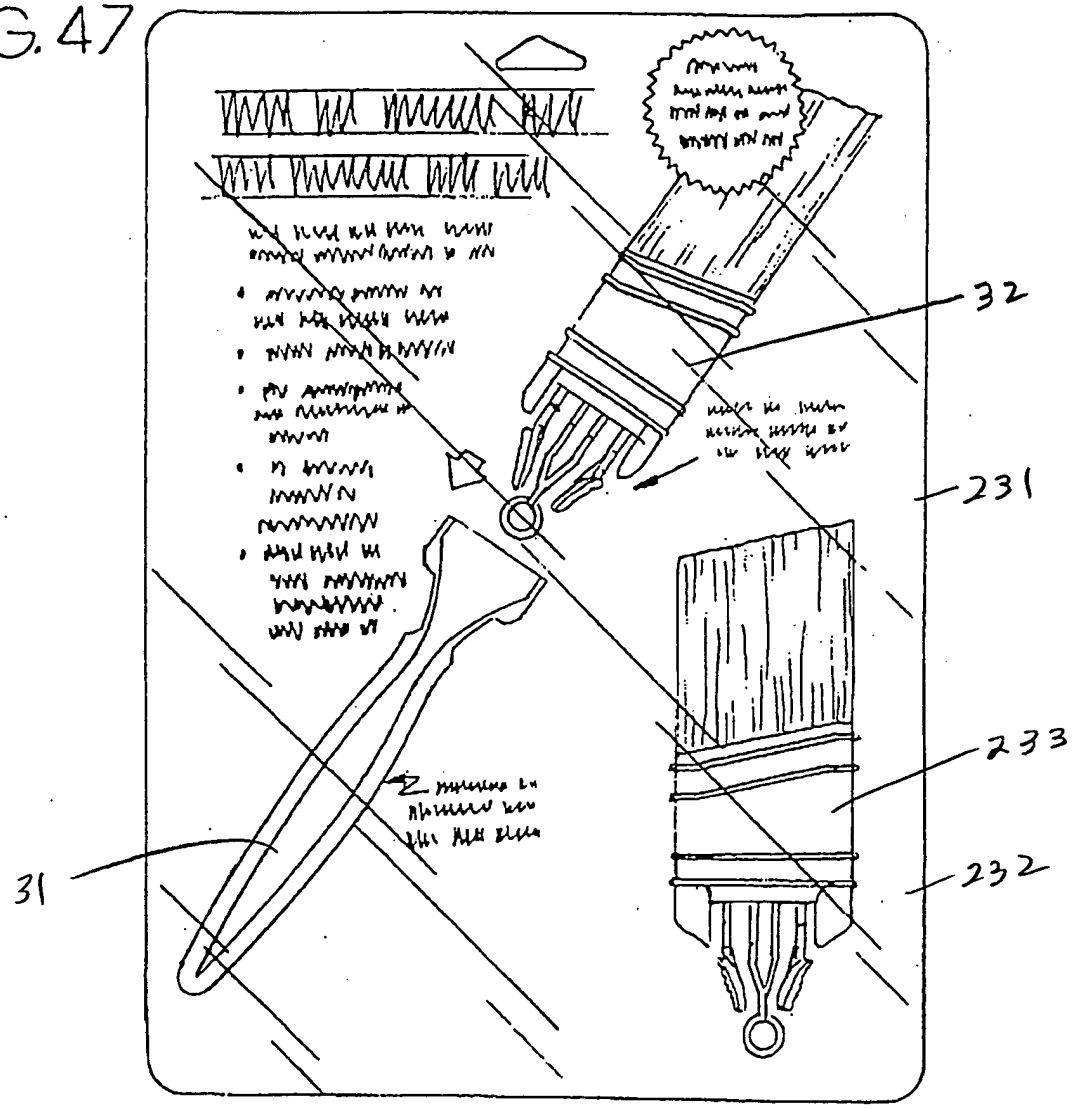


FIG. 48

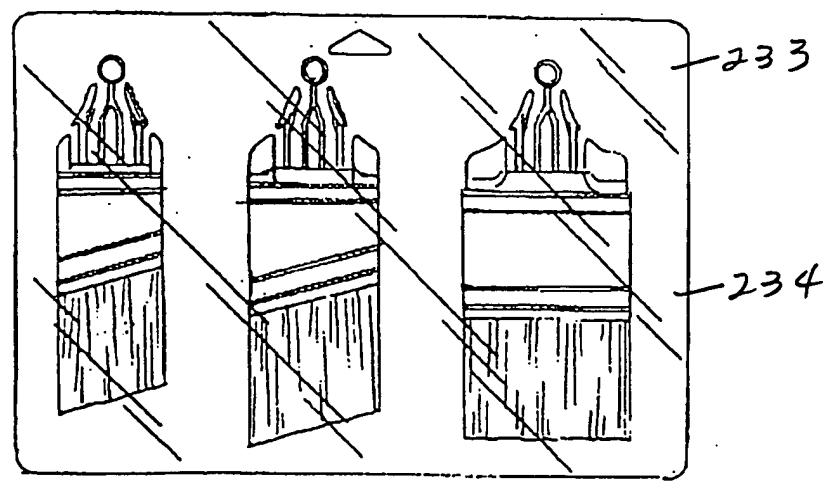


FIG. 49

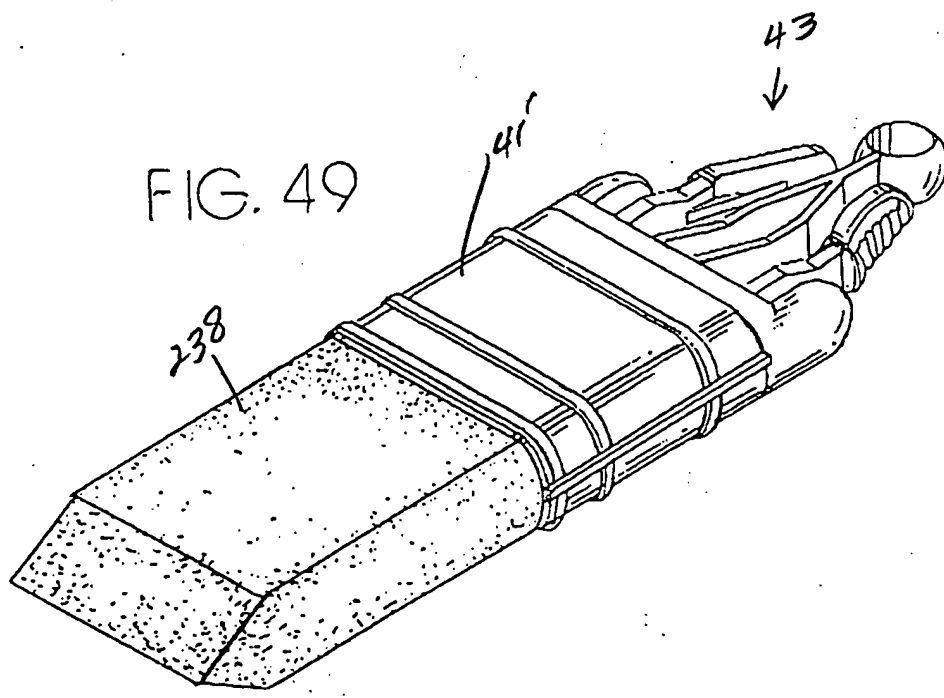


FIG. 50

